


Sample Information

Name :生物素三肽-1
Sequence :Biotin-GHK
Pump A :0.1%Trifluoroacetic in 100% water
Pump B :0.1%Trifluoroacetic in 100% acetonitrile
Total Flow :1ml/min
Wavelength :214nm
Analytical column type :Phenomenex Luna® 5 µm C18(2) (4.6*250mm*5 µm)
Dissolution method :100%H2O
Inj. Volume : 25ul
Time Module Action Value
0.01 Pumps B.Conc 5
25.00 Pumps B.Conc 30
33.00 Pumps B.Conc 100
38.00 Pumps B.Conc 100
40.00 Pumps B.Conc 5
50.00 Controller Stop

Chromatogram

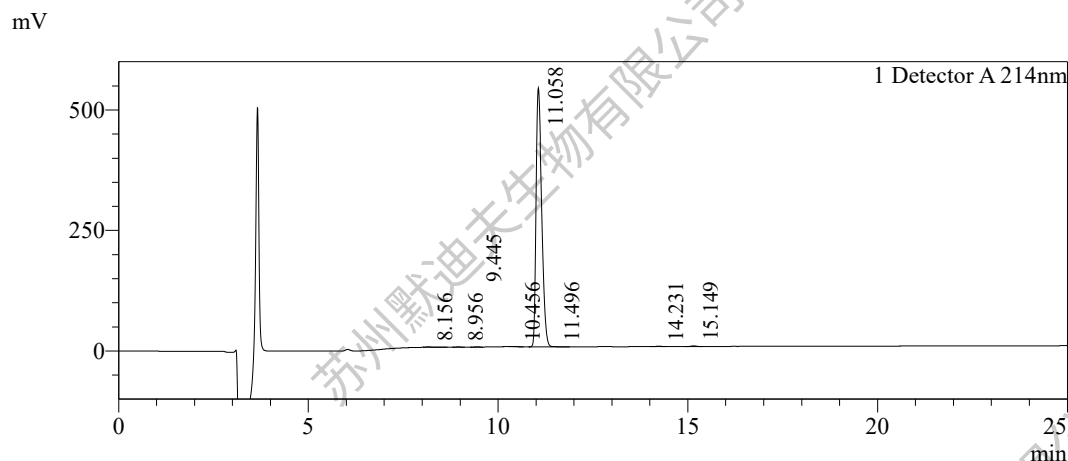

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	8.156	10183	577	0.178
2	8.956	3089	367	0.054
3	9.445	3136	386	0.055
4	10.456	5675	553	0.099
5	11.058	5681734	537478	99.199
6	11.496	3323	350	0.058
7	14.231	8351	834	0.146
8	15.149	12096	1332	0.211
Total		5727588	541877	100.000

邮箱: marketing@motifbiotech.com

网址: http://www.motifbiotech.com

地址: 苏州市高新区浒墅关镇浒青路111号B04