


MS Spectrum

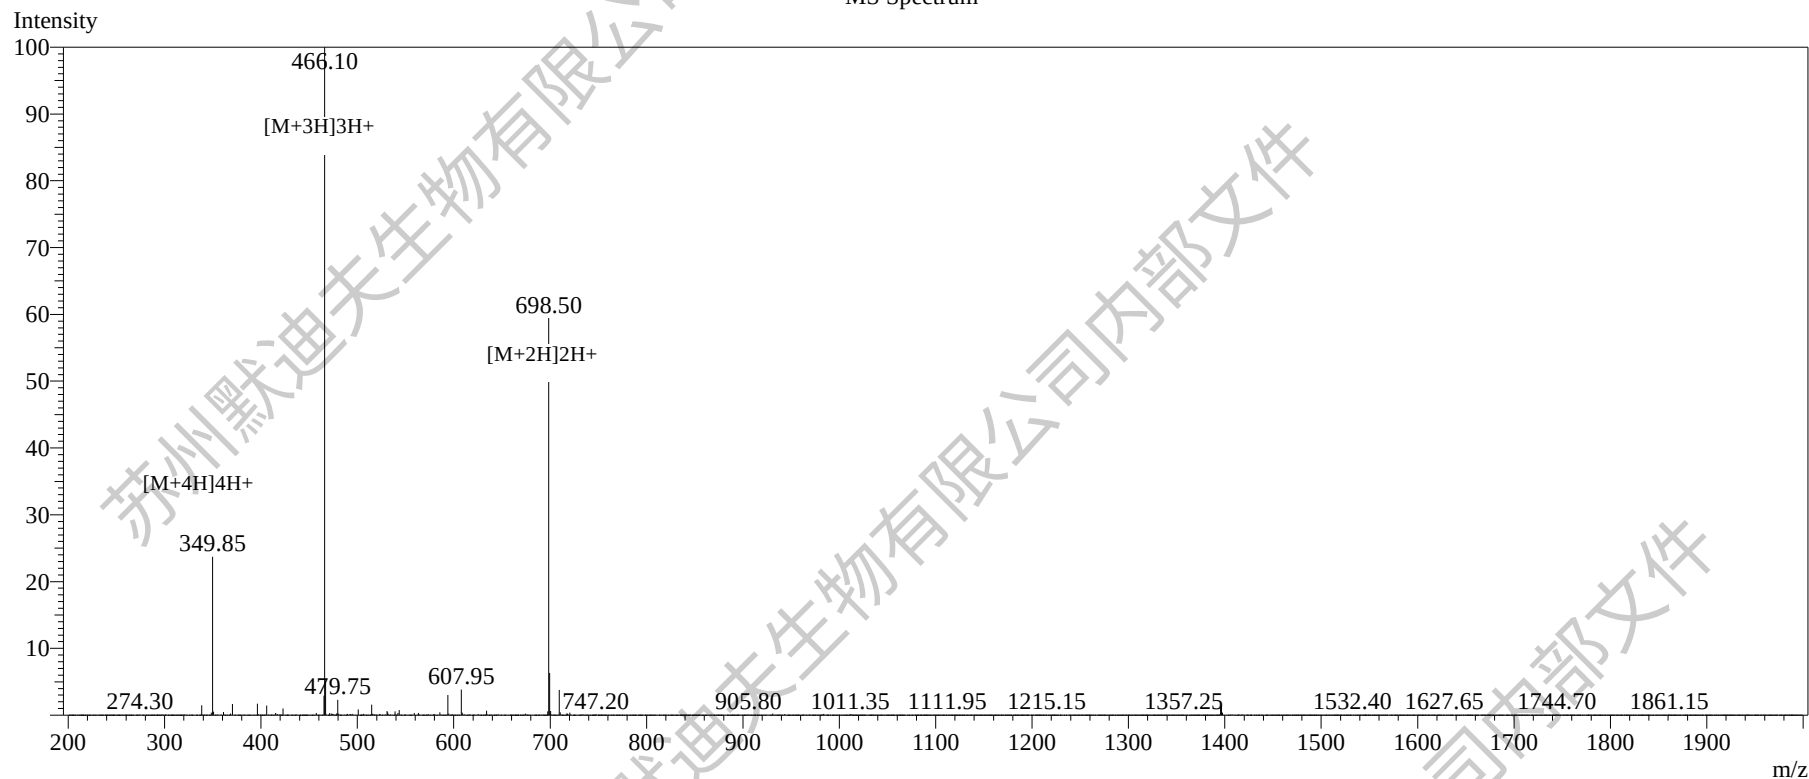

Sample Information

Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/09/26 11:20:35	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

Name : 十肽-12
 Sequence : YRSRKYSSWY (Acetate Salt)
 Theoretical : 1395.52
 Observed : 1395.30

邮箱: marketing@motifbiotech.com

网址: <https://www.motifbiotech.com>

地址: 苏州市高新区浒墅关镇浒青路111号B04