


MS Spectrum

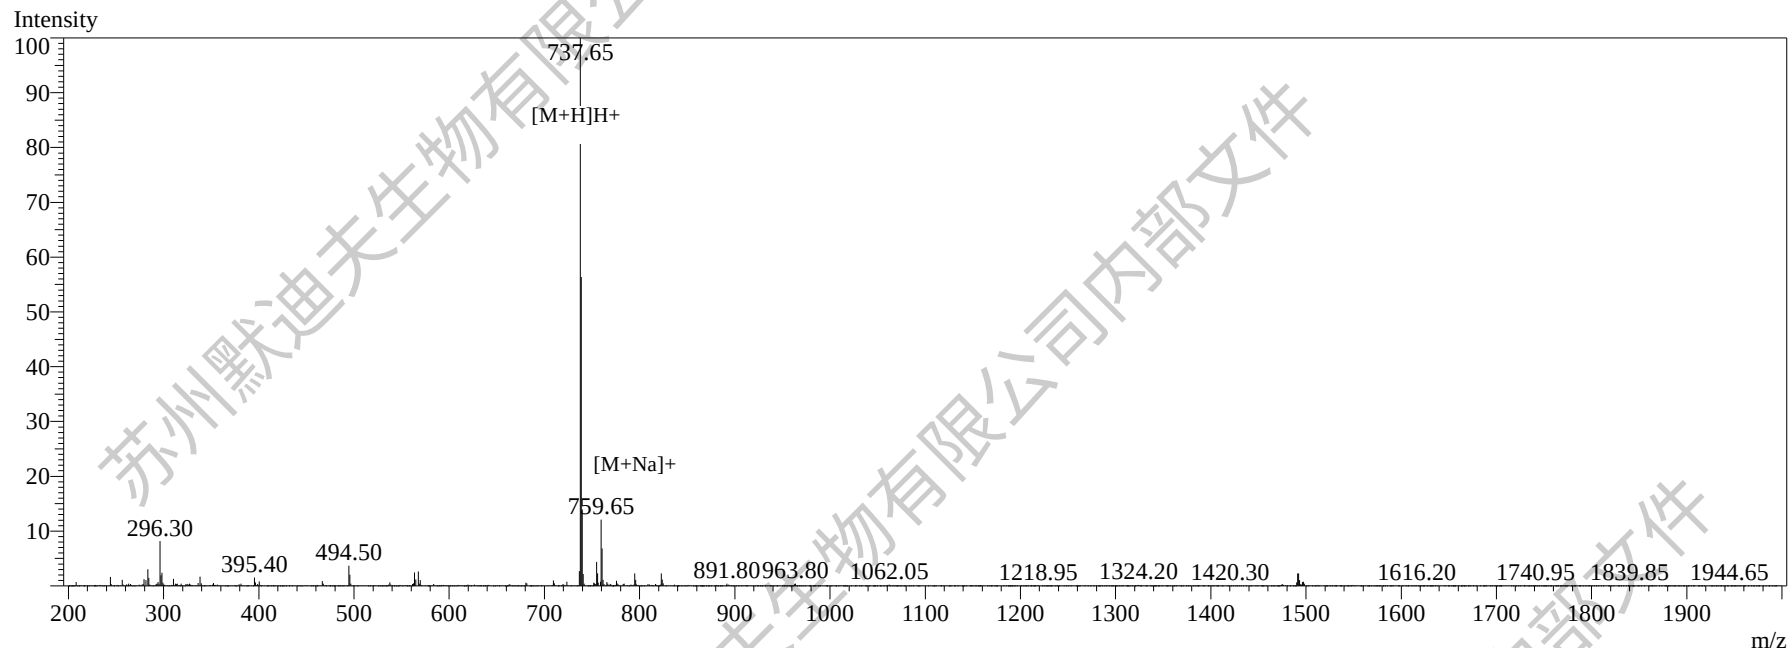

Sample Information

Dissolution method :15%ACN+85%H₂O
Date Acquired :2024/04/23 16:43:48
Injection Volume :0.2ul
Block Temp :200

Interface :ESI
Nebulizing Gas Flow :1.50L/min
CDL Temp :250°C
CDL Volt :0v

Prerod Bias :+4.5kv
Detector :-0.2kv
T.Flow :0.2ml/min
B.conc :50%H₂O/50%MEOH

Name :棕榈酰六肽-12
Sequence :Pal-VGVAPG
Theoretical :736.98
Observed :736.65

邮箱 : marketing@motifbiotech.com

网址 : <https://www.motifbiotech.com>

地址 : 苏州市高新区浒墅关镇浒青路111号B04